biovo technologies

EN

Airway Medix Oral Care

INSTRUCTIONS FOR USE

1.1. INDICATION FOR USE

These instructions are intended for use with the following products:

B-Care Toothbrush
#32200
4ml Pipette
#PE

Before operating **B-CARE TOOTHBRUSH** please read these instructions and save this manual for future reference.

1.2. IMPORTANT

- This product is not intended for use by children.

- Use this product only for its intended use as described in this manual. Do not use accessories not recommended by the manufacturer.

1.3. INTENDED USE

- This product is not intended for use by children.

- The B-Care is a toothbrush intended to maintain a good oral hygiene, including plaque removal. The product includes the toothbrush and two pipettes for liquids loading.

1.4. WARNING

• The product is not intended for use by children.

• Handle and store properly DO NOT disassemble the product.

• DO NOT use if packaging has been damaged.

• Device must be used only for the intended purpose.

• Non-sterile. DO NOT attempt to sterilize or autoclave this product.

• Do not use the product if any parts show signs of damage. This may cause injury.

• The product is intended for single use only

2. DESCRIPTION

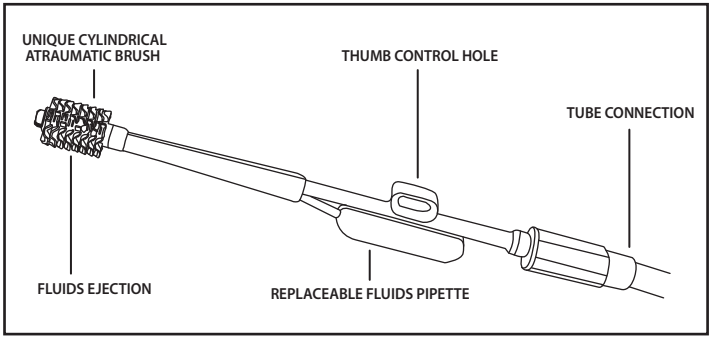

3. B-CARE OPERATION INSTRUCTIONS

3.1. Insert the Pipette to load cleaning liquids [Figure 1].

3.2. Connect the Pipette to the brush [Figure 2].



Figure 1

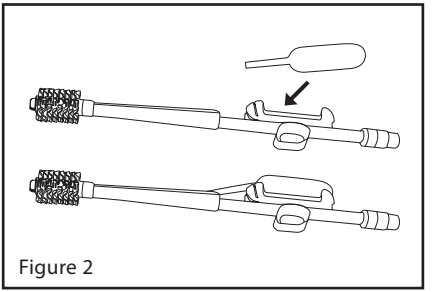

Figure 2

3.3. Hold the brush with thumb on Thumb Control Hole and finger on the Pipette. Apply liquids by gently press on the Pipette [Figure 3].

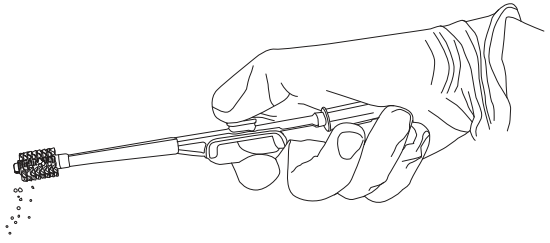

Figure 3

4. GUARANTEE

We grant 2 years guarantee on the product commencing on date of purchase. Within the guarantee period we will eliminate, free of charge, any defects in the appliance resulting from faults in materials or workmanship, either by repairing or replacing the complete appliance as we may choose.

This guarantee does not cover: damage due to improper use, normal wear or use, defects that have a negligible effect on the value or operation of the appliance. The guarantee becomes void if repairs are undertaken by unauthorized persons and if original Biovo Technologies parts are not used. To obtain service within the guarantee period, hand in or send the complete appliance with your sales representative.

Biovo Technologies Ltd.
23rd HaMelacha Street, POB 11419
Park Afek, Rosh-HaAyin, 4809173, Israel
Tel: (+972) 72-2151115 | **Fax:** (+972) 72-2151112
Email: info@biovo-tech.com

Manufactured for:
Airway Medix S.A.
ul. Gen. Józefa Zajączka 11/14, 01-510 Warsaw, Poland
Tel: +48 22 408 44 80 | **Email:** info@airwaymedix.pl
Assembled and packed in the UK

002-06-LAB Rev.00